

DAKEWE



HP300 Automatic tissue processor

Tissue processing well managed

HP300 Tissue Processor

Reliability

Self-diagnostics

Automatically check key parameters upon startup and before the process starts, minimizing the possibility of malfunction from the beginning

Component monitoring

Real-time monitoring of components and parameter settings. Together with intelligent analysis and precaution, further offers great overall performances

Temperature control

Multi-point temperature sensors and intelligent control algorithm spontaneously provide excellent temperature control

Safety

Remote monitoring

Remote monitoring of errors to increase instrument uptime, alert via multiple methods when a risk is detected

Ceramic rotary valve

Heat-resistant ceramic valve significantly reduces blockage caused by wax attachment and thus promotes the stability and accuracy of liquid delivery

Ultrasonic sensors


3 ultrasonic sensors in the retort unaffected by wax build-ups are able to provide correct liquid level information consistently

Workflow improving

Multi-dimensional reagent management


Multi-dimensional monitoring of reagent usage, reagent replenishment record can be generated and exported for lab statistics

Consumption can be recorded in cassettes, cycles and days

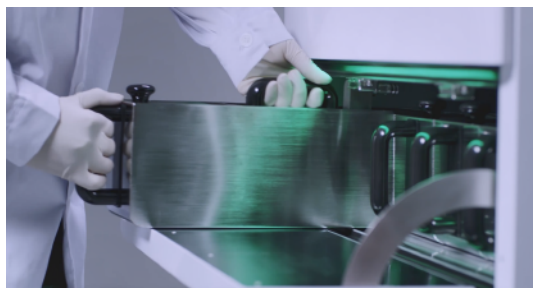

Tissue processing well managed

Dakewe HP300 tissue processor

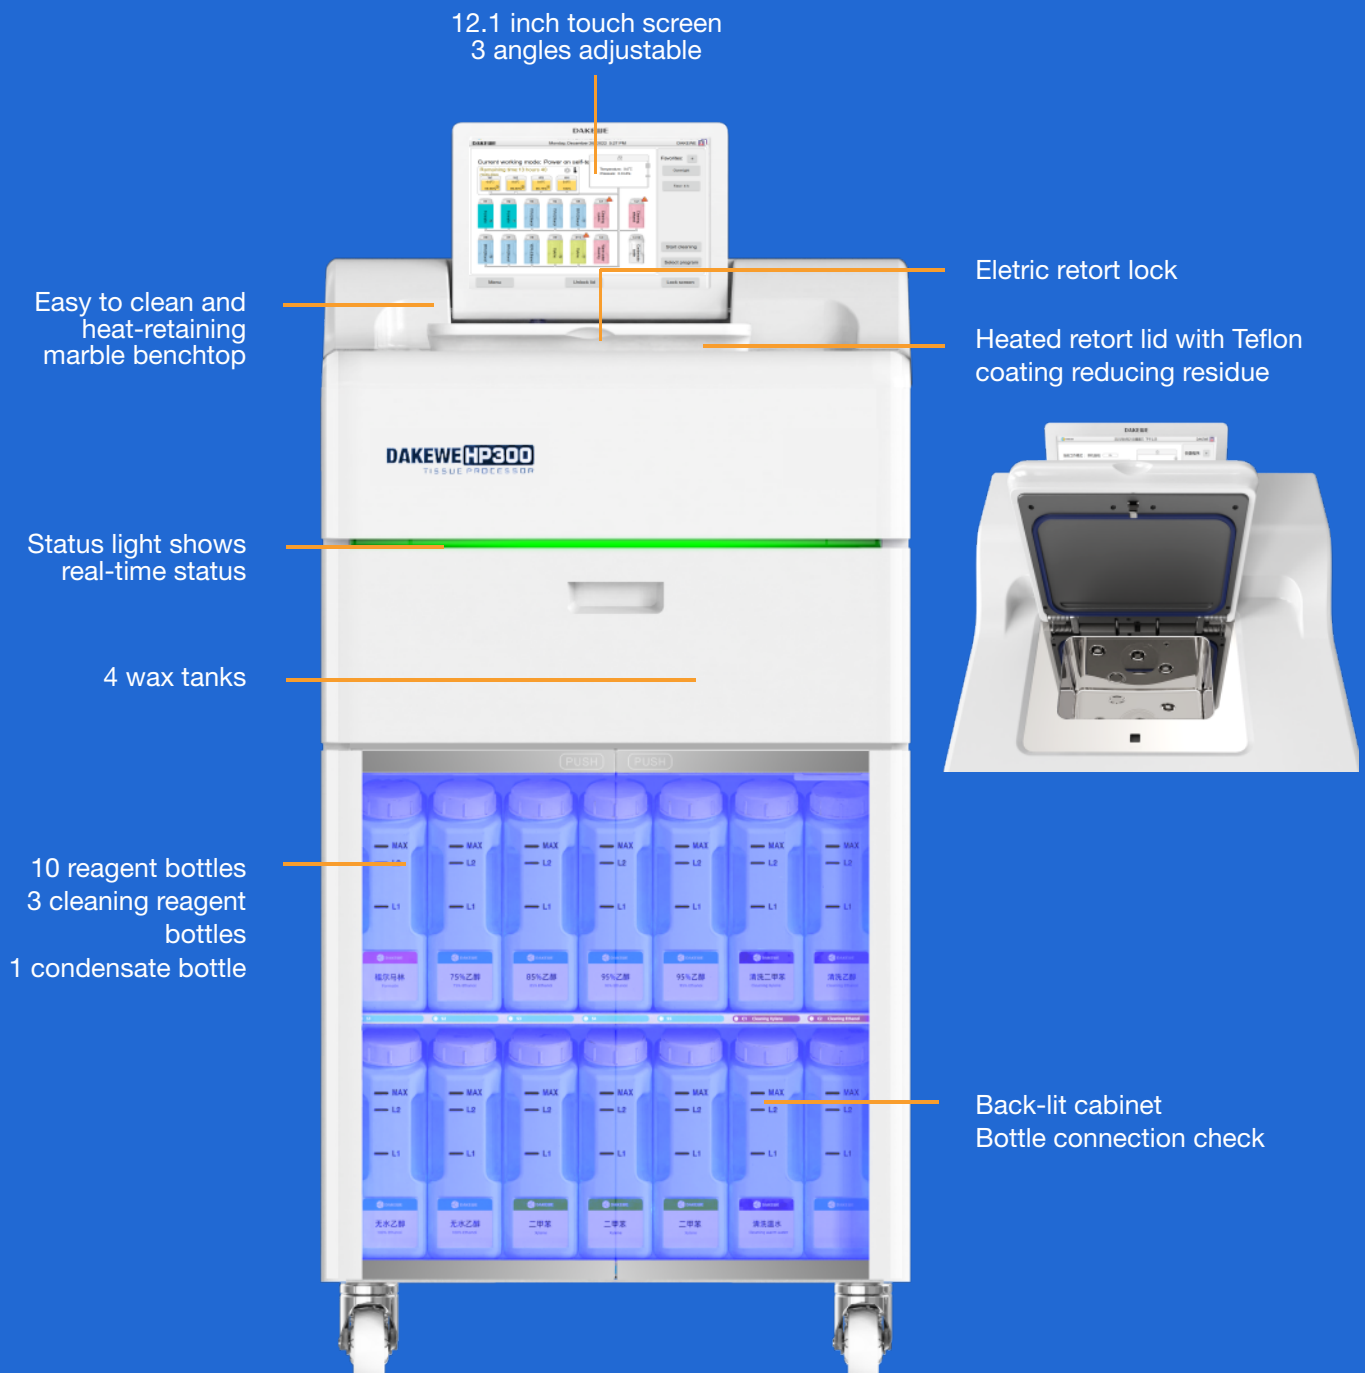

Specifications

Process capacity	Up to 300 cassettes in 2 large baskets, or 280 in 4 small baskets
Wax tanks	3 × 4.2 L, 1 × 5.6 L
Reagent bottles	10 reagent bottles, 3 cleaning reagent bottles, 1 condensate bottle
Program memory	Up to 100 programs
Level sensors	3 ultrasonic level sensors
Screen	12.1 inch LCD color touch screen, 3 angles adjustable
Data interface	USB, LAN
Power	100 - 120 VAC, 60 Hz or 220 - 240 VAC, 50/60 Hz; 1200 VA
Dimensions (W×D×H)	620 × 640 × 1170 mm
Weight	Approx. 180 kg, without reagents

DAKEWE

Dakewe medical
Shenzhen, China
www.dakewemedical.com
Ver 3.0, Rev. July 2024

